
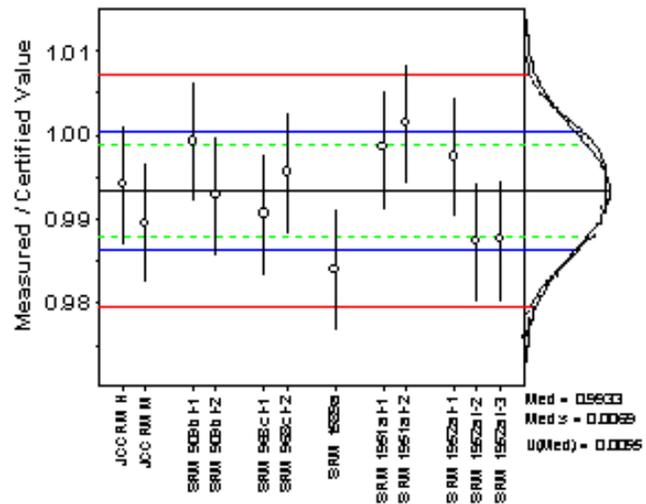


Figure 1.

Comparison of "higher order" Cholesterol in Serum CRMs

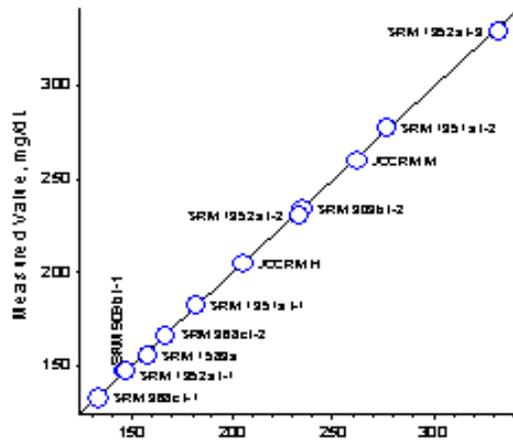

⇒ CRM comparability independent of analyte level

The measured/certified ratios for this set of CRMs are:

- ~ normally distributed
- with a standard deviation of ~0.7%